



Sea-Bird GmbH

Postfach 1167, 87401 Kempten, Germany

Phone: +49 831 9 60994 701 Fax: +49 831 960994 709

Email: seabird.eu@seabird.com

Conductivity Calibration Report

Customer:	EMS/Spain		
Job Number:	E00966	Date of Report:	11/4/2015
Model Number:	SBE 04C	Serial Number:	043513

Conductivity sensors are normally calibrated 'as received', without cleaning or adjustments, allowing a determination of sensor drift. If the calibration identifies a problem or indicates cell cleaning is necessary, then a second calibration is performed after work is completed. The 'as received' calibration is not performed if the sensor is damaged or non-functional, or by customer request.

An 'as received' calibration certificate is provided, listing the coefficients used to convert sensor frequency to conductivity. Users must choose whether the 'as received' calibration or the previous calibration better represents the sensor condition during deployment. In SEASOFT enter the chosen coefficients. The coefficient 'slope' allows small corrections for drift between calibrations (consult the SEASOFT manual). Calibration coefficients obtained after a repair or cleaning apply only to subsequent data.

'AS RECEIVED CALIBRATION'

Performed Not Performed

Date: 10/20/2015

Drift since last cal: 0.00000 PSU/month*

Comments:

'FINAL CALIBRATION'

Performed Not Performed

Date: 11/4/2015

Drift since 06 Sep 12 -0.00010 PSU/month*

Comments:

**Measured at 3.0 S/m*

Cell cleaning and electrode replatinizing tend to 'reset' the conductivity sensor to its original condition. Lack of drift in post-cleaning-calibration indicates geometric stability of the cell and electrical stability of the sensor circuit.

Sea-Bird GmbH

Postfach 1167, 87401 Kempten, Germany

Phone: +49 831 960994 701 Fax: +49 831 960994 709 Email: seabird.eu@seabird.com

SENSOR SERIAL NUMBER: 3513
CALIBRATION DATE: 04-Nov-15

SBE 4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

COEFFICIENTS:

g = -1.01569686e+001
h = 1.22297669e+000
i = -1.69050149e-003
j = 1.71929390e-004

CPcor = -9.5700e-008 (nominal)
CTcor = 3.2500e-006 (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.88593	0.00000	0.00000
-1.0000	34.8257	2.80526	5.59887	2.80525	-0.00001
1.0000	34.8262	2.97673	5.72307	2.97674	0.00000
15.0000	34.8266	4.27274	6.58595	4.27278	0.00004
18.5000	34.8266	4.61959	6.79813	4.61956	-0.00002
29.0000	34.8240	5.70344	7.42183	5.70341	-0.00003
32.5000	34.8124	6.07539	7.62399	6.07541	0.00002

f = INST FREQ / 1000.0

Conductivity = $(g + h * f^2 + i * f^3 + j * f^4) / (1 + \delta * t + \epsilon * p)$ Siemens / meter

t = temperatur e[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = instrument conductivity - bath conductivity

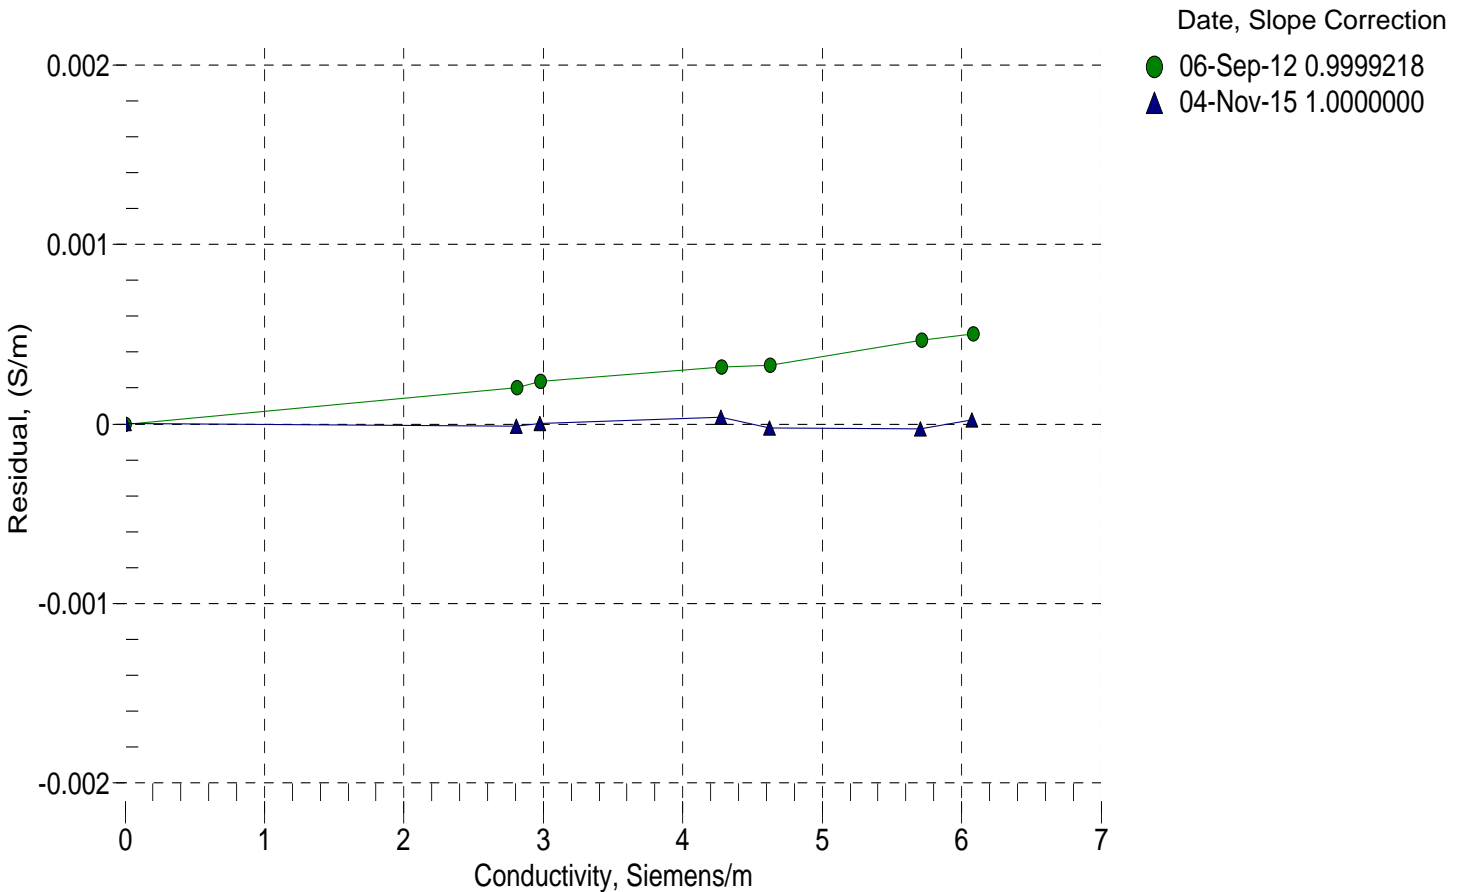

Sea-Bird GmbH

Postfach 1167, 87401 Kempten, Germany

Phone: +49 831 960994 701 Fax: +49 831 960994 709 Email: seabird.eu@seabird.com

SENSOR SERIAL NUMBER: 3513
CALIBRATION DATE: 20-Oct-15

SBE 4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

COEFFICIENTS:

g = -1.01575606e+001
h = 1.22298766e+000
i = -1.65529132e-003
j = 1.66165887e-004

CPcor = -9.5700e-008 (nominal)
CTcor = 3.2500e-006 (nominal)


BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.88594	0.00000	0.00000
-1.0001	34.7998	2.80336	5.59748	2.80338	0.00002
1.0000	34.8008	2.97477	5.72163	2.97474	-0.00002
15.0000	34.8012	4.26996	6.58424	4.26995	-0.00001
18.5000	34.8005	4.61650	6.79638	4.61653	0.00003
29.0000	34.7967	5.69947	7.41981	5.69943	-0.00004
32.5000	34.7878	6.07158	7.62215	6.07161	0.00002

f = INST FREQ / 1000.0

Conductivity = (g + h * f² + i * f³ + j * f⁴) / (1 + δ * t + ε * p) Siemens / meter

t = temperatur [°C]; p = pressure[decibars]; δ = CTcor; ε = CPcor;

Residual = instrument conductivity - bath conductivity

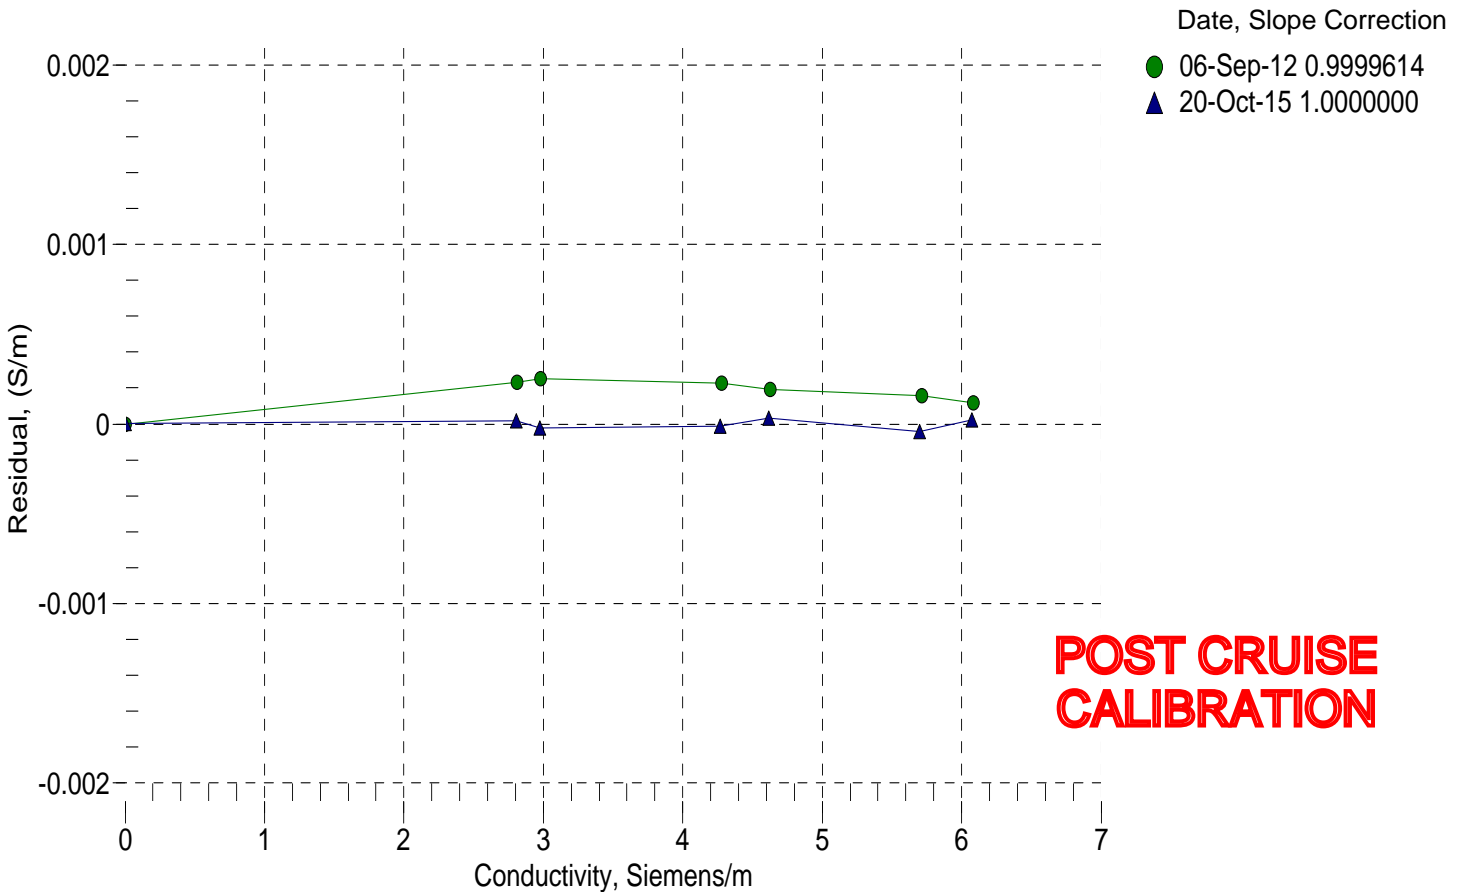



Sea-Bird GmbH
Postfach 1167, 87401 Kempten, Germany
Phone: +49 831 9 60994 701 Fax: +49 831 960994 709
Email: seabird.eu@seabird.com

Pressure Test Certificate

Customer EMS/Spain
Job Number E00966
Date 11/11/2015
Technician TK

Serial Number 043513

Low Pressure (PSI) 45 PSI
Time (Minutes) 15 Minutes

High Pressure (PSI) 8000 PSI
Time (Minutes) 30 Minutes

Pass
Fail

Comments

Replaced the main piston "O"-Rings.

